




Hygromatic II

PRODUCT OVERVIEW

GENERAL SPECIFICATIONS - Hygromatic II

CALIBRATION TO	TRANSFER STANDARD	No Charge			
(17025 TRACEABLE TO NIST)	CERTIFICATE	17025 Validation (Additional Fees Apply)			
OPERATING AMBIENT CONDI-	TEMPERATURE	18 °C to 28 °C			
TIONS	HUMIDITY	Up to 80 % RH			
STORAGE CONDITIONS	TEMPERATURE	-20 °C to 50 °C			
STORAGE CONDITIONS	HUMIDITY	0 % to 95 % RH (non-condensing)			
ALTITUDE	2000 m				
CALIBRATION SYSTEM ACCURACY	TEMPERATURE	± 0.10 °C Or Better Typical	y ± 0.05 °C	*Based on Probe Accuracy	
	HUMIDITY	± 1.00 % RH Or Better Special	y tuned systems can be as good as \pm 0.60 $\%$	*Based on Probe Accuracy	
	CONTROLLER TYPE	PID Controller			
		0.10 °C Or Better Typically ± 0.05 °C			
	HUMIDITY	0.30 % RH @ 18 °C to 28 °C Or Better Typically \pm 0.25 %			
STABILITY	TEMPERATURE	0.05 °C			
STADILITT	HUMIDITY	0.15 % RH @ 18 °C to 28 °C			
WARM-UP PERIOD	AMBIENT CONDITIONS		30 Minutes Maximum		
	COLD	30 Minutes			
RESOLUTION		Temperature	0.01 °C		
	DISPLAY	Humidity	0.01 % RH		
		Dew Point	0.01 °C (Calculated)		
	USB	Temperature	0.01 °C		
		Humidity	0.01 % RH		

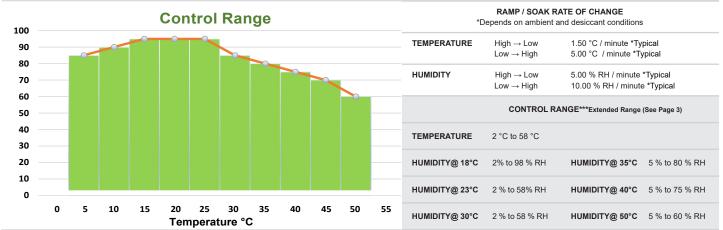

CONSUMABLES

	RESERVOIR	200 ml	
	RESERVOIR	200 111	
WATER	SPILL RESISTANT	Yes	
	REQUIRED FLUID	Distilled Water Only	
	EST. REFILL PERIOD	15 Days to 1 Month (Typical) *Depends on Usage	
	FILL INDICATOR	Floating Ball	
DESICCANT	ТҮРЕ	Molecular Sieve	
	REPLACEMENT	When Indicating Desiccant is 3/4 Used	
	REPLACEMENT FREQUENCY	Depends Entirely on User Workload	
	LOCATION	Left Side Mounted	
	FASTENER	Desiccant Mounting Bracket Provided	
RECALIBRATION	FREQUENCY	Depends on User Uncertainty Requirements	
		Once Per Year Recommended	

**Information subject to change, please visit our website for updates at www.geocalibration.com.

MECHANICAL

GENERATOR DIMENSIONS	Measurement Type	Width	Depth	Height
	Metric	55.33 cm	40.65 cm	24.65 cm
	English	21.78 in	16.02 in	9.70 in
CHAMBER DIMENSIONS	Measurement Type	Diameter	Depth	
	Metric	14.50 cm	20.00 cm	
	English	5.71 in	7.87 in	
	Measurement Type	Diameter	Depth	
WORKING DIMENSIONS AND VOLUME	Metric	12.50 cm	10.90 cm	
WORKING DIMENSIONS AND VOLUME	English	4.92 in	4.29 in	
	Volume	1.5 Liter Effective Working Volume		
WEIGHT	Unit Only	Metric	15.5 kg	
WEIGHT		English	34.0 lb	
POWER SUPPLY		12 Volt DC @ 1A		
STANDARD PORT QUANTITY	Depends on doors	Availability: 6 Ports, 5 Ports, 4 Ports, 2 Ports		
	•			
CHILLED MIRROR PORTS	In and Out			
CHILLED MIRROR PORTS	In and Out		Probe Range	Actual Unit Range
				Actual Unit Range + 5.00 to + 60.00 °C
CHILLED MIRROR PORTS PROBE ANALOG OUTPUTS AVAILABLE	In and Out 0 - 1 Volt	Temperature	Probe Range	

*** Extended Ranges for Temperature and Humidity

Upon users request GEO is Offering the extended ranges for both Temperature and Humidity which are as following:

EXTENDED CONTROL RANGE			
TEMPERATURE	2 °C to 58 °C (Normal is 5 °C to 55 °C)	HUMIDITY@ 35°C	2 % to 80 % RH (Normal is 5% to 80%)
HUMIDITY@ 18°C	2 % to 95 % RH (Normal is 5% to 95%)	HUMIDITY@ 40°C	2 % to 75 % RH (Normal is 5% to 75%)
HUMIDITY@ 23°C	2% to 98% RH(Normal is 5% to 95%)	HUMIDITY@ 50°C	2 % to 60 % RH (Normal is 5% to 60%)
HUMIDITY@ 30°C	2 % to 85 % RH (Normal is 5% to 85%)		

1. The Temperature ranges are not guaranteed if the environment Temperature is not controlled to 23 °C. User will see stable and extended results if environmental temperature is controlled at 23 °C or 72 °F. The normal temperature working ranges in Model 2000SP are 18 °C to 28 °C for different Humidity ranges. The Extended Ranges can help the user to test Hygrometers for lower or higher temperature values, although for Rh it may not be a great use at the extended temperature ranges.

2. The Humidity ranges are affected by the temperature especially for the high humidity above 70%. On high humidity if the temperature drops, it can go to Dew Point and can form the Condensation. To prevent condensation, user must bring the temperature to desired value first and then bring the Humidity to desired value. The extended Rh ranges are offered for the Hygrometers that needed to be calibrated below 5% or above 95%. It will not get the best calibration tolerances because the probe goes out of linear range.

Note: To go to the lower Rh, such as 2%, user must make sure the Desiccant is reasonably good. For high Rh, such as 98%, user have to use the insulated door only.

3. The following table shows the order how user should set the set points to get the best results without getting the Dew Point condition or Condensation, avoiding the unnecessary use of Desiccant and make the system more efficient.

Table Temperature vs Humidity relationship and how to get the best result:

Temperature	Humidity
NO Change	Set Rh Hi/LO within Specification Range
Low to High	Set Rh Hi/LO within Specification Range
High to Low	If Rh is Higher than 70%, Set Rh to 70% first. Set the temperature to desired value and then Set Rh to desired value within Specification Range

* Complete Accessory List is Available at www.geocalibration.com

**Information subject to change, please visit our website for updates at www.geocalibration.com.



Humidity Control Company



Proudly Made in the USA

Email: Sales@GeoCalibration.com Website: www.GeoCalibration.com